

EXHIBIT G-2
THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY A.A.C. R13-10-104 (A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY
STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000

STANDARD CALIBRATION CHECK PROCEDURE

QA SPECIALIST J. ROGERS AGENCY GOODYEAR P.D.
DATE 11-2-06 TIME 1736
INTOXILYZER SERIAL # 80-000312 LOCATION GOODYEAR P.D.

1. Ensure that gas tank is attached to instrument and contains a standard alcohol concentration solution, 100 AC.
OR
Pour a standard alcohol concentration solution _____ AC, into a clean dry simulator and assemble the simulator. Ensure that a tight seal has been made. Turn on the simulator and allow temperature to reach $34^{\circ}\text{C} \pm 0.2^{\circ}\text{C}$
2. Intoxilyzer 8000 display reads "PUSH BUTTON TO START"
3. Go to the "Control Testing Menu". Select "D" for dry control test or "W" for wet control test. After selection is made press ENTER.
4. Air blank completed.
5. Calibration check completed. Test results 0.099 AC.
6. Air blank completed.
7. Remove printed record. Attach the record to the completed checklist.

SIGNATURE _____

J. Rogers #1123

DPS Form Exh G-2 (Rev 05-01)

END OF LOT 432401I

INTOXILYZER 8000

Location: GOODYEAR POLICE DEPT

Serial Number: 80-000312

11/02/2006

17:36:42

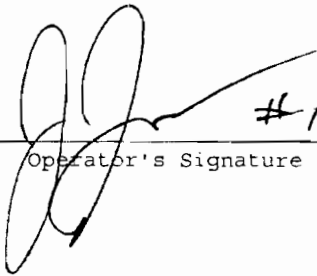
Standard Lot#: 432401I

Last Changed By: J. VALLANDINGHAM #981

QAS: J. ROGERS #1123

GOODYEAR PD

Test	g/210L	Time
Air Blank	0.000	17:37:09
Cal Check	0.099	17:37:28
Air Blank	0.000	17:37:58



Operator's Signature #1123

END OF LOT

EXHIBIT G-2
THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY A.A.C. R13-10-104 (A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY
STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000

STANDARD CALIBRATION CHECK PROCEDURE

QA SPECIALIST J. ROGERS AGENCY GOODYEAR P.D.
DATE 11-2-06 TIME _____
INTOXILYZER SERIAL # 80-000312 LOCATION GOODYEAR P.D.

1. Ensure that gas tank is attached to instrument and contains a standard alcohol concentration solution _____ AC.
OR
Pour a standard alcohol concentration solution _____ AC, into a clean dry simulator and assemble the simulator. Ensure that a tight seal has been made. Turn on the simulator and allow temperature to reach $34^{\circ}\text{C} \pm 0.2^{\circ}\text{C}$
2. Intoxilyzer 8000 display reads "PUSH BUTTON TO START"
3. Go to the "Control Testing Menu". Select "D" for dry control test or "W" for wet control test. After selection is made press ENTER.
4. Air blank completed.
5. Calibration check completed. Test results 0. _____ AC.
6. Air blank completed.
7. Remove printed record. Attach the record to the completed checklist.

SIGNATURE [Signature] #1123

DPS Form Exh G-2 (Rev 05-01)

START OF LOT 618601I
EXP 7-7-08

INTOXILYZER 8000

Location: GOODYEAR POLICE DEPT

Serial Number: 80-000312

11/02/2006

17:43:31


Standard Lot#: 618601I

Last Changed By: J. ROGERS #1123

QAS: J. ROGERS #1123

GOODYEAR PD

Test	g/210L	Time
Air Blank	0.000	17:43:58
Cal Check	0.101	17:44:17
Air Blank	0.000	17:44:46

 # 1123

Operator's Signature



Scott Specialty Gases, Inc.

CERTIFICATE OF ANALYSIS EBS™ - Ethanol Breath Standard

Customer Name
CMI
316 East Ninth Street
Owensboro, KY 42303

Assay Laboratory
Scott Specialty Gases
6141 Easton Road, Bldg. 1
Plumsteadville, Pa. 18949

Purchase Order: 370201
Scott Project # 0153910
Lot No.: 618101G
Expiration Date:
July 5, 2008

<u>REFERENCE STANDARD</u>	<u>CYLINDER #</u>	<u>CONCENTRATION ppm</u>
N.I.S.T. Traceable Standards*	ALM-059986	103.2
	ALM-060143	118.1
	ALM-060196	223.2
	ALM-037475	302.0

CONTAINER TYPE: 28

LOT CERTIFIED VALUE CONCENTRATION

<u>COMPONENTS</u>	<u>ppm (BrAC)</u>	<u>ACCURACY</u>
Ethanol	117.2 (0.045)	+/- 2%
Nitrogen	Balance	

*Certification: Traceable to N.I.S.T. RGM Ethanol Standards

Analyst:

Date: 07/07/2006

EXHIBIT G-2
THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY A.A.C. R13-10-104 (A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY
STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000

STANDARD CALIBRATION CHECK PROCEDURE

QA SPECIALIST J. ROGERS AGENCY GOODYEAR P.D.
DATE 11-22-06 TIME 1554
INTOXILYZER SERIAL # 80-000312 LOCATION GOODYEAR P.D.

- 1. Ensure that gas tank is attached to instrument and contains a standard alcohol concentration solution, 100 AC.
OR
Pour a standard alcohol concentration solution _____ AC, into a clean dry simulator and assemble the simulator. Ensure that a tight seal has been made. Turn on the simulator and allow temperature to reach $34^{\circ}\text{C} \pm 0.2^{\circ}\text{C}$
- 2. Intoxilyzer 8000 display reads "PUSH BUTTON TO START"
- 3. Go to the "Control Testing Menu". Select "D" for dry control test or "W" for wet control test. After selection is made press ENTER.
- 4. Air blank completed.
- 5. Calibration check completed. Test results 0. 100 AC.
- 6. Air blank completed.
- 7. Remove printed record. Attach the record to the completed checklist.

SIGNATURE [Signature] #1123

DPS Form Exh G-2 (Rev 05-01)

INTOXILYZER 8000

Location: GOODYEAR POLICE DEPT

Serial Number: 80-000312

11/22/2006

15:54:51


Standard Lot#: 618601I

Last Changed By: J. ROGERS #1123

QAS: J. ROGERS #1123

GOODYEAR PD

Test	g/210L	Time
Air Blank	0.000	15:55:18
Cal Check	0.100	15:55:37
Air Blank	0.000	15:56:07

 #1123

Operator's Signature