

EXHIBIT 2

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY A.A.C. R9-14-404(A)

ARIZONA DEPARTMENT OF HEALTH SERVICES

STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000

STANDARD CALIBRATION CHECK PROCEDURE

AGENCY GOODYEAR POLICE DEPARTMENT

DATE _____ TIME _____

INTOXILYZER SERIAL NO. 80-000312 LOCATION GOODYEAR PD

QA SPECIALIST Will
(print name)

W 1. Ensure dry gas tank is attached to instrument and contains a known alcohol standard 100 AC.

OR

Pour a standard alcohol solution of known value, _____ AC, into a clean dry simulator and assemble the simulator. Ensure that a tight seal has been made. Turn on the simulator and allow temperature to reach $34^{\circ}\text{C} \pm 0.2^{\circ}\text{C}$

W 2. Intoxilyzer 8000 display reads "PUSH BUTTON TO START"

W 3. Go to the "Control Testing Menu". Select "D" for dry control test or "W" for wet control test. After selection is made press ENTER.


W 4. Air blank completed.

W 5. Calibration check completed. Test results 0. 099 AC.

W 6. Air blank completed.

W 7. Remove printed record. Attach the record to the completed checklist.

SIGNATURE: _____




INTOXILYZER 8000
Location: GOODYEAR POLICE DEPT
Serial Number: 80-000312
09/10/2005 02:27:09

Standard Lot#: 431001G
Last Changed By: W. WILL #974

QAS: W. WILL #974
GOODYEAR PD

Test	g/210L	Time
Air Blank	0.000	02:27:37
Cal Check	0.099	02:27:55
Air Blank	0.000	02:28:25

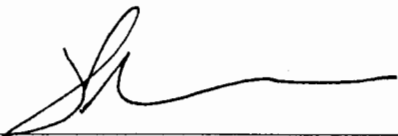

Operator's Signature

GAS CYLINDER
CHANGE

431001G

EXHIBIT 2

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY A.A.C. R9-14-404(A)

ARIZONA DEPARTMENT OF HEALTH SERVICES

STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000

STANDARD CALIBRATION CHECK PROCEDURE

AGENCY GOODYEAR POLICE DEPARTMENT
DATE _____ TIME ~~07~~ 0222
INTOXILYZER SERIAL NO. 80-000312 LOCATION GOODYEAR PD
QA SPECIALIST Will
(print name)

- W1. Ensure dry gas tank is attached to instrument and contains a known alcohol standard 100 AC.
- OR
- Pour a standard alcohol solution of known value, 0.097 AC, into a clean dry simulator and assemble the simulator. Ensure that a tight seal has been made. Turn on the simulator and allow temperature to reach $34^{\circ}\text{C} \pm 0.2^{\circ}\text{C}$
- W2. Intoxilyzer 8000 display reads "PUSH BUTTON TO START"
- W3. Go to the "Control Testing Menu". Select "D" for dry control test or "W" for wet control test. After selection is made press ENTER.
- W4. Air blank completed.
- W5. Calibration check completed. Test results 0. 097 AC.
- W6. Air blank completed.
- W7. Remove printed record. Attach the record to the completed checklist.

SIGNATURE: _____

INTOXILYZER 8000

Location: GOODYEAR POLICE DEPT

Serial Number: 80-000312

09/10/2005

02:21:35


Standard Lot#: 422601G

Last Changed By: W. WILL #974

QAS: W. WILL #974

GOODYEAR PD

Test	g/210L	Time
Air Blank	0.000	02:22:03
Cal Check	0.097	02:22:21
Air Blank	0.000	02:22:51

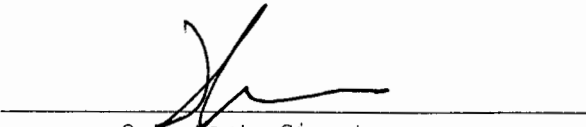

Operator's Signature



Scott Specialty Gases, Inc.

43101G

CERTIFICATE OF ANALYSIS EBS™ - Ethanol Breath Standard

Customer Name
CMI
316 East Ninth Street
Owensboro, KY 42303

Assay Laboratory
Scott Specialty Gases
6141 Easton Road, Bldg. 1
Plumsteadville, Pa.
18949-0310

Purchase Order : 367651
Scott Project #: 0119378
Lot No.: 431001G
Expiration Date:
November 8, 2006

REFERENCE STANDARD	CYLINDER #	CONCENTRATION ppm
N.I.S.T. Traceable Standards*	ALM-060154	103.6
	ALM-060204	118.1
	ALM-059962	222.2
	ALM-037472	251.0

CONTAINER TYPE: 105

LOT CERTIFIED VALUE

CONCENTRATION

COMPONENTS	ppm (BrAC)	ACCURACY
Ethanol	260.5 (0.100)	+/- 2%
Nitrogen	Balance	

*Certification: Traceable to N.I.S.T. RGM Ethanol Standards

Floyd Bard

Analyst:

Date: 11/23/2004