

EXHIBIT G-2
THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY A.A.C. R13-10-104 (A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY
STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000

STANDARD CALIBRATION CHECK PROCEDURE

QA SPECIALIST JEFF ROGERS AGENCY GOODYEAR P.D.
DATE 9-16-07 TIME 1809
INTOXILYZER SERIAL # 80-001858 LOCATION GOODYEAR PD

- (✓) 1. Ensure that gas tank is attached to instrument and contains a standard alcohol concentration solution 100 AC.
OR

Pour a standard alcohol concentration solution _____ AC, into a clean dry simulator and assemble the simulator. Ensure that a tight seal has been made. Turn on the simulator and allow temperature to reach $34^{\circ}\text{C} \pm 0.2^{\circ}\text{C}$

- (✓) 2. Intoxilyzer 8000 display reads "PUSH BUTTON TO START"
(✓) 3. Go to the "Control Testing Menu". Select "D" for dry control test or "W" for wet control test. After selection is made press ENTER.
(✓) 4. Air blank completed.
(✓) 5. Calibration check completed. Test results 0. 099 AC.
(✓) 6. Air blank completed.
(✓) 7. Remove printed record. Attach the record to the completed checklist.

SIGNATURE [Signature] #1123

DPS Form Exh G-2 (Rev 05-01)

LOT 536401I
EXP 1-3-08

INTOXILYZER 8000

Location: GOODYEAR POLICE DEPT

Serial Number: 80-001858

09/16/2007

18:09:12


Standard Lot#: 536401I

Last Changed By: M. SLONEKER #6559

QAS: J. ROGERS #1123

GOODYEAR PD

Test	g/210L	Time
Air Blank	0.000	18:09:39
Cal Check	0.099	18:09:58
Air Blank	0.000	18:10:28

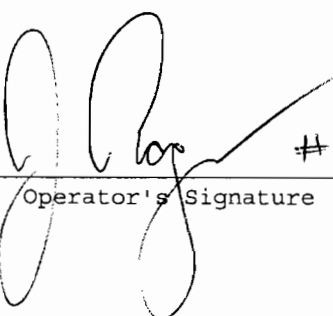 #1123

Operator's Signature

EXHIBIT G-4
THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY A.A.C. R13-10-104 (A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY
STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000

STANDARD QUALITY ASSURANCE PROCEDURE

QA SPECIALIST JEFF ROGERS AGENCY GOODYEAR PD
DATE 9-16-07 TIME 1812
INTOXILYZER SERIAL # 80-001858 LOCATION GOODYEAR PD

(☒) 1. Display Reads "PUSH BUTTON TO START"

DIAGNOSTIC TESTS

- (☒) 1. Clock time check.
(☒) 2. Date check.

OPERATIONAL TESTS

- (☒) 1. Alcohol-free subject test result 0. 00 AC.
(☒) 2. Error recognition logic system functioning.
Not a Successfully Completed Test Sequence printed
(☒) 3. Proper sample recognition system.
Not a Successfully Completed Test Sequence printed
Deficient sample printed.
(☒) 4. Standard Calibration Check standard 0. 100 AC. Result 0. 098 AC.

Instrument is operating properly and accurately. YES ☒ NO ☐

COMMENTS

SIGNATURE [Signature] #1123

LOT 536401I
EXP 1-3-08

INTOXILYZER 8000

Location: GOODYEAR POLICE DEPT

Serial Number : 80-001858

09/16/2007

18:12:21

Standard Lot#: 536401I

Last Changed By: M. SLONEKER

#6559

QAS: J. ROGERS

#1123

GOODYEAR PD

Operator: J. ROGERS

#1123

GOODYEAR PD

Subject: TEST,TEST

DOB: 01/01/0101

Sex: M

Weight: 100

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	18:13:30
Diagnostic Test	Pass	18:13:57
Air Blank	0.000	18:14:24
0.100 Cal Check	0.099	18:14:43
Air Blank	0.000	18:15:13
Subject Test	0.000	18:15:31
Air Blank	0.000	18:15:58
Five Minute Wait	ABT*	
Air Blank	0.000	18:16:37

*Sequence Aborted

Not a Successfully Completed Test Sequence

INTOXILYZER 8000

Location: GOODYEAR POLICE DEPT

Serial Number : 80-001858

09/16/2007

18:17:07

Standard Lot#: 536401I

Last Changed By: M. SLONEKER #6559

QAS: J. ROGERS #1123

GOODYEAR PD

Operator: J. ROGERS #1123

GOODYEAR PD

Subject: TEST,TEST

DOB: 01/01/0101

Sex: M

Weight: 100

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	IPS*	18:17:49
Air Blank	0.000	18:18:18

*Improper Sample

Not a Successfully Completed Test Sequence

INTOXILYZER 8000

Location: GOODYEAR POLICE DEPT

Serial Number : 80-001858

09/16/2007

18:18:39

Standard Lot#: 536401I

Last Changed By: M. SLONEKER

#6559

QAS: J. ROGERS

#1123

GOODYEAR PD

Operator: J. ROGERS

#1123

GOODYEAR PD

Subject: TEST,TEST

DOB: 01/01/0101

Sex: M

Weight: 100

15 Minute Deprivation Period? Yes

Test	<u>g/210L</u>	Time
Air Blank	RFI*	18:19:18
Air Blank	0.000	18:19:47

*RFI Detect

USED NEXTEL D/C

Not a Successfully Completed Test Sequence

INTOXILYZER 8000

Location: GOODYEAR POLICE DEPT

Serial Number : 80-001858

09/16/2007

18:20:20

Standard Lot#: 536401I

Last Changed By: M. SLONEKER

#6559

QAS: J. ROGERS

#1123

GOODYEAR PD

Operator: J. ROGERS

#1123

GOODYEAR PD

Subject: TEST,TEST

DOB: 01/01/0101

Sex: M

Weight: 100

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	18:21:08
Diagnostic Test	Pass	18:21:36
Air Blank	0.000	18:22:03
0.100 Cal Check	0.100	18:22:22
Air Blank	0.000	18:22:52
Subject Test	0.024*	18:26:00
Air Blank	0.000	18:26:30
Air Blank	0.000	18:26:57
Subject Test	XXX**	18:27:52
Air Blank	0.000	18:28:25

*Deficient Sample

**Invalid Sample

Begin new deprivation period

Not a Successfully Completed Test Sequence

EXHIBIT G-2
THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY A.A.C. R13-10-104 (A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY
STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000

STANDARD CALIBRATION CHECK PROCEDURE

QA SPECIALIST JEFF ROGERS AGENCY GOODYEAR P.D.
DATE 9-16-07 TIME 1829
INTOXILYZER SERIAL # 80-001858 LOCATION GOODYEAR P.D.

- (☒) 1. Ensure that gas tank is attached to instrument and contains a standard alcohol concentration solution, 100 AC.
OR
Pour a standard alcohol concentration solution _____ AC, into a clean dry simulator and assemble the simulator. Ensure that a tight seal has been made. Turn on the simulator and allow temperature to reach $34^{\circ}\text{C} \pm 0.2^{\circ}\text{C}$
- (☒) 2. Intoxilyzer 8000 display reads "PUSH BUTTON TO START"
- (☒) 3. Go to the "Control Testing Menu". Select "D" for dry control test or "W" for wet control test. After selection is made press ENTER.
- (☒) 4. Air blank completed.
- (☒) 5. Calibration check completed. Test results 0. 098 AC.
- (☒) 6. Air blank completed.
- (☒) 7. Remove printed record. Attach the record to the completed checklist.

LOT 536401Z
EXP 1-3-08

SIGNATURE [Signature] #1123

INTOXILYZER 8000

Location: GOODYEAR POLICE DEPT

Serial Number: 80-001858

09/16/2007

18:29:06


Standard Lot#: 536401I

Last Changed By: M. SLONEKER #6559

QAS: J. ROGERS #1123

GOODYEAR PD

Test	g/210L	Time
Air Blank	0.000	18:29:34
Cal Check	0.098	18:29:52
Air Blank	0.000	18:30:22

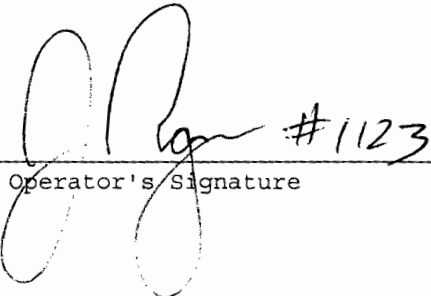

Operator's Signature