

Intoxilyzer - Alcohol Analyzer  
Model 9000

SN: 90-003795

Test Date: 05/07/2023

Test Time: 04:41

Location: 11 N 145TH AVENUE

Software Version: 9439.01.00

Standard Lot #: 18022100A2

Standard Value: 0.100

Expiration Date: 09/05/2024

Bottle #: 003

Last Changed By: MIYAZATO, KORY

Permit #: 30215

Operator: MIYAZATO, KORY


Permit #: 30215

Agency: GOODYEAR PD

Test	g/210L	Time
Air Blank	0.000	04:42:06
Calibration Chk	0.097	04:42:27
Air Blank	0.000	04:43:07

No RFI Detected

Successfully Completed Test Sequence

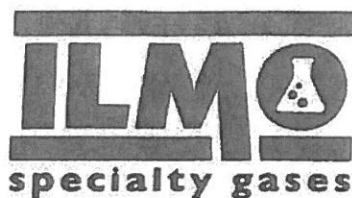

7 Eastgate Dr. • P.O. Box 790 • Jacksonville, IL 62651-0790  
217-245-2183 • Fax: 217-243-7634 • www.ilmoproducts.com

## Certificate of Analysis

**Certificate ID:** 14918  
**Part #:** BAC105L100T  
**Cylinder Size:** 105L  
**Lot Number:** 18022100A2  
**Expiration:** 9/5/2024

0.100 BAC (For the calibration of instruments used to determine breath alcohol concentration)

**Contents:** 105 Liters @ 1000 psig 70°F (21°C)

Component:	Reported Concentration:	Analytical	
		Accuracy (U, k=2):	Analytical Method:
Ethanol	260 ppm	+/-0.002 BAC(G/210L)	NDIR
Nitrogen	Balance	[5.2 ppm]	

**Distributed by:**

CMI Inc.  
316 East Ninth Street  
Owensboro, KY 42303  
Phone 866-835-0690  
[www.alcoholtest.com](http://www.alcoholtest.com)

\*Traceable to:  
NIST Research Gas Mixture - 212.6 µmol/mol  
Ethanol in Nitrogen - Serial No. SA15944

Store in dry area, away from sources of heat, ignition and direct sunlight. Do not allow storage area to exceed 52 °C (125 °F).

*Christopher Wright*  
Specialty Gas Lab Tech

8-8-2022  
Issuance Date



Calibration results within this certificate were obtained at the facility listed above using equipment and standards capable of producing analytical results traceable to NIST, and apply to the items contained on this certificate. ILMO Products Company makes no warranty or representation as to the suitability of the use of any information provided for any particular use. The information use is at the sole discretion and risk of the user. Liability shall be limited to established replacement cost of this material or service. This certificate applies only to items described and shall not be reproduced other than in full, without written approval from the issuing facility.



Intoxilyzer - Alcohol Analyzer  
Model 9000

SN: 90-003795

Test Date: 05/24/2023

Test Time: 04:29

Location: 11 N 145TH AVENUE

Software Version: 9439.01.00

Standard Lot #: 18022100A2

Standard Value: 0.100

Expiration Date: 09/05/2024

Bottle #: 003

Last Changed By: MIYAZATO, KORY

Permit #: 30215

Operator: MIYAZATO, KORY

Permit #: 30215

Agency: GOODYEAR PD

Test	g/210L	Time
Air Blank	0.000	04:29:31
Calibration Chk	0.100	04:29:52
Air Blank	0.000	04:30:32

No RFI Detected



ARIZONA DEPARTMENT OF PUBLIC SAFETY  

---

INTOXILYZER MAINTENANCE REPORT

CR NO. I900037950003

Page 1 of 1

**AGENCY** Goodyear Police Department  
Goodyear, AZ 85338  
**OFFICER** MIYAZATO, #1139  
**DATE** May 26, 2023



**INSTRUMENT**

90003795

**INSTRUMENT LOCATION**

Goodyear Police Department

**MAINTENANCE REQUESTED**

Repair

**MAINTENANCE PERFORMED**

*Erin E Boone*

---

ERIN E. BOONE, #5823, Forensic Scientist  
Central Regional Crime Laboratory  
2102 W. Encanto Blvd., Phoenix, AZ 85009  
602-223-2281 eboone@azdps.gov

EXHIBIT I-2

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY A.A.C. R13-10-104 (A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY  
INTOXILYZER MODEL 9000

PERIODIC MAINTENANCE AND STANDARD QUALITY ASSURANCE PROCEDURE

QA SPECIALIST K Miyazato 1139 AGENCY Goodyear  
DATE 5/30/23 TIME 2120  
INTOXILYZER SERIAL# 90-003795

1. Ensure that gas tank is attached and contains a standard alcohol concentration 100 AC

DIAGNOSTIC TESTS

- 1. Clock time check
- 2. Date check

OPERATIONAL TESTS

- 1. Deficient Subject Test (Proper Sample Recognition)  
Deficient Sample printed
- 2. Alcohol-free Subject Test (Proper Sample Recognition):  
0.000 AC
- 3. Mouth Alcohol Subject Test (Proper Sample Recognition):  
Invalid Sample – Begin new deprivation period printed
- 4. Radio Frequency Interference Test (Error Recognition):  
RFI Detect printed
- 5. Standard Calibration Check:  
0.098 AC
- 6. Air Blanks Completed
- 7. Timer Reset

Not a Successfully Completed Test Sequence will be printed

Instrument is operating properly and accurately. YES  NO

COMMENTS:

\_\_\_\_\_  
\_\_\_\_\_  
\_\_\_\_\_

SIGNATURE

K Miyazato 1139

# ARIZONA FORENSIC BREATH ALCOHOL ANALYTICAL REPORT

11 N 145TH AVENUE

## INSTRUMENT INFORMATION

Analytical Instrument: Intoxilyzer 9000  
Serial Number: 90-003795  
Software Version: 9439.01.00  
Analytical Report Number: 37950530230322

QAS: MIYAZATO, KORY  
QAS Permit #: 30215  
Agency: GOODYEAR PD  
Last 31-Day Check: 05/30/2023  
Last Annual Maintenance: 08/03/2022

## SUBJECT INFORMATION

Name: 31-Day Check  
Test Date: 05/30/2023  
Driver's License #:  
Gender:  
Date of Birth:  
Age:

Weight:  
State of Issue:  
Driver's License Expiration:  
Deprivation Start Time: 21:00  
15 - Minute Deprivation: Yes

## OPERATOR INFORMATION

Name: MIYAZATO, KORY  
Agency: GOODYEAR PD

Permit #: 30215

## STANDARD INFORMATION

Standard Value: 0.100  
Standard Lot #: 18022100A2  
Expiration Date: 09/05/2024  
Bottle #: 003  
Last Changed By: MIYAZATO, KORY

Permit #: 30215

## RESULTS

Test	g/210L	Time
Air Blank	0.000	21:20:37
Diagnostic Test	PASS	21:21:13
Air Blank	0.000	21:21:49
Calibration Chk	0.099	21:22:11
Air Blank	0.000	21:22:50
Subject Test 1	NSG*	21:26:05
Air Blank	0.000	21:26:46
Air Blank	0.000	21:27:27
Subject Test 2	0.000	21:27:44
Air Blank	0.000	21:28:25
Wait		21:32:28
Air Blank	0.000	21:33:05
Subject Test 3	INV**	21:33:21
Air Blank	RFI***	21:33:37

\*No Sample Given

\*\*Invalid Sample - Begin new deprivation period

\*\*\*RFI Detect

## EXCEPTION MESSAGES

\* No Sample Given

\*\* Invalid Sample - Begin new deprivation period

\*\*\* RFI Detect

## OPERATOR COMMENTS

All air blank results must be 0.000.

Consecutive subject test results must not differ by more than 0.020 g/210L.

Standard check results must be  $\pm 10\%$ .

Not a Successfully Completed Test Sequence

Intoxilyzer - Alcohol Analyzer  
Model 9000

SN: 90-003795

Test Date: 05/30/2023

Test Time: 21:34

Location: 11 N 145TH AVENUE

Software Version: 9439.01.00

Standard Lot #: 18022100A2

Standard Value: 0.100

Expiration Date: 09/05/2024

Bottle #: 003

Last Changed By: MIYAZATO, KORY

Permit #: 30215

Operator: MIYAZATO, KORY

Permit #: 30215

Agency: GOODYEAR PD

Test	g/210L	Time
Air Blank	0.000	21:34:31
Calibration Chk	0.098	21:34:53
Air Blank	0.000	21:35:32

No RFI Detected



# ARIZONA FORENSIC BREATH ALCOHOL ANALYTICAL REPORT

11 N 145TH AVENUE

## INSTRUMENT INFORMATION

Analytical Instrument: Intoxilyzer 9000  
Serial Number: 90-003795  
Software Version: 9439.01.00  
Analytical Report Number: 37950530230321

QAS: MIYAZATO, KORY  
QAS Permit #: 30215  
Agency: GOODYEAR PD  
Last 31-Day Check: 04/29/2023  
Last Annual Maintenance: 08/03/2022

## SUBJECT INFORMATION

Name: 31-Day Check  
Test Date: 05/30/2023  
Driver's License #:  
Gender:  
Date of Birth:  
Age:

Weight:  
State of Issue:  
Driver's License Expiration:  
Deprivation Start Time: 21:00  
15 - Minute Deprivation: Yes

## OPERATOR INFORMATION

Name: MIYAZATO, KORY  
Agency: GOODYEAR PD

Permit #: 30215

## STANDARD INFORMATION

Standard Value: 0.100  
Standard Lot #: 18022100A2  
Expiration Date: 09/05/2024  
Bottle #: 003  
Last Changed By: MIYAZATO, KORY

Test	g/210L	Time
Air Blank	0.000	21:18:48
Diagnostic Test	DIA*	21:18:54
Air Blank	0.000	21:19:31

\*00004000000  
IRPCM Status Error

Permit #: 30215

## RESULTS

## EXCEPTION MESSAGES

\* Diagnostic Fail

## OPERATOR COMMENTS

No RFI Detected

All air blank results must be 0.000.  
Consecutive subject test results must not differ by more than 0.020 g/210L.  
Standard check results must be  $\pm 10\%$ .

Not a Successfully Completed Test Sequence